ANALIZA BIAŁEK

100013609

Laboratory of Analysis

Client: Anonymous
Order number: 100013609
Name: REVIVA+ GHK
Number of samples: 1 vial

Batch number: ------
Receive date: 2026-03-23
Start date: 2026-03-28
Enda date: 2026-05-04

Sample identification

Substance	Method of taking a sample	Form
GHK-Cu	Sample provided by customer	Blue liquid in glass vial

Results

Substance	Sample name	Content	Purity
GHK-Cu	REVIVA+ GHK	17,82mg/ml 53,46mg/3ml	99%
GHK-Cu	REVIVA+ GHK AFTER 1 MONTH IN ROOM TEMPERATURE	17,70mg/ml 53,10mg/3ml	99%

Research comment

The test sample was applied in the amount of 3µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H20 and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peaks of the sought substances appeared. Its concentration, when compared to the reference chromatogram shows the table above. Height the measurement error is + - 0,05 mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample



Password

7W54S2MH

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875


Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając


ANALIZA BIAŁEK

100013609

Chromatogram

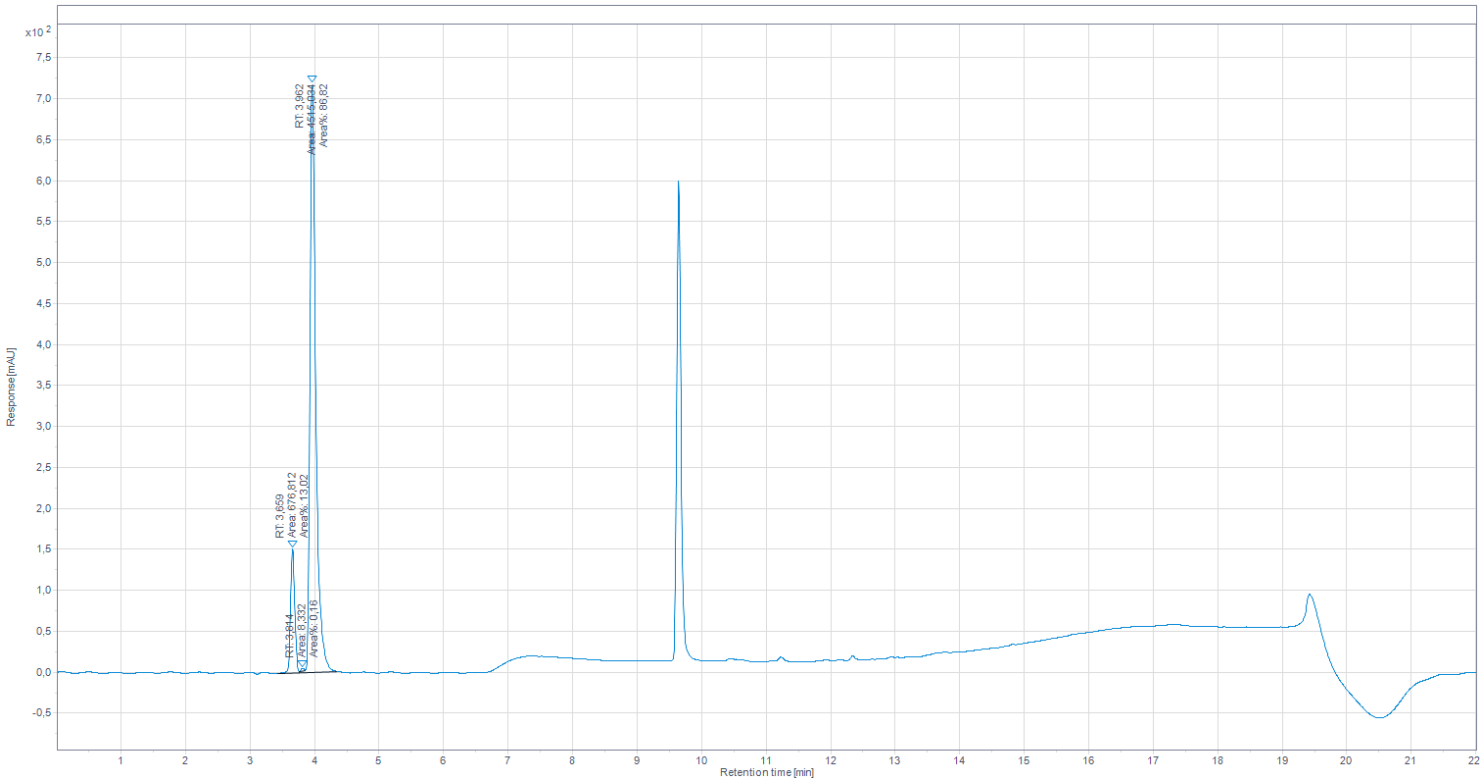

Chromatogram 2

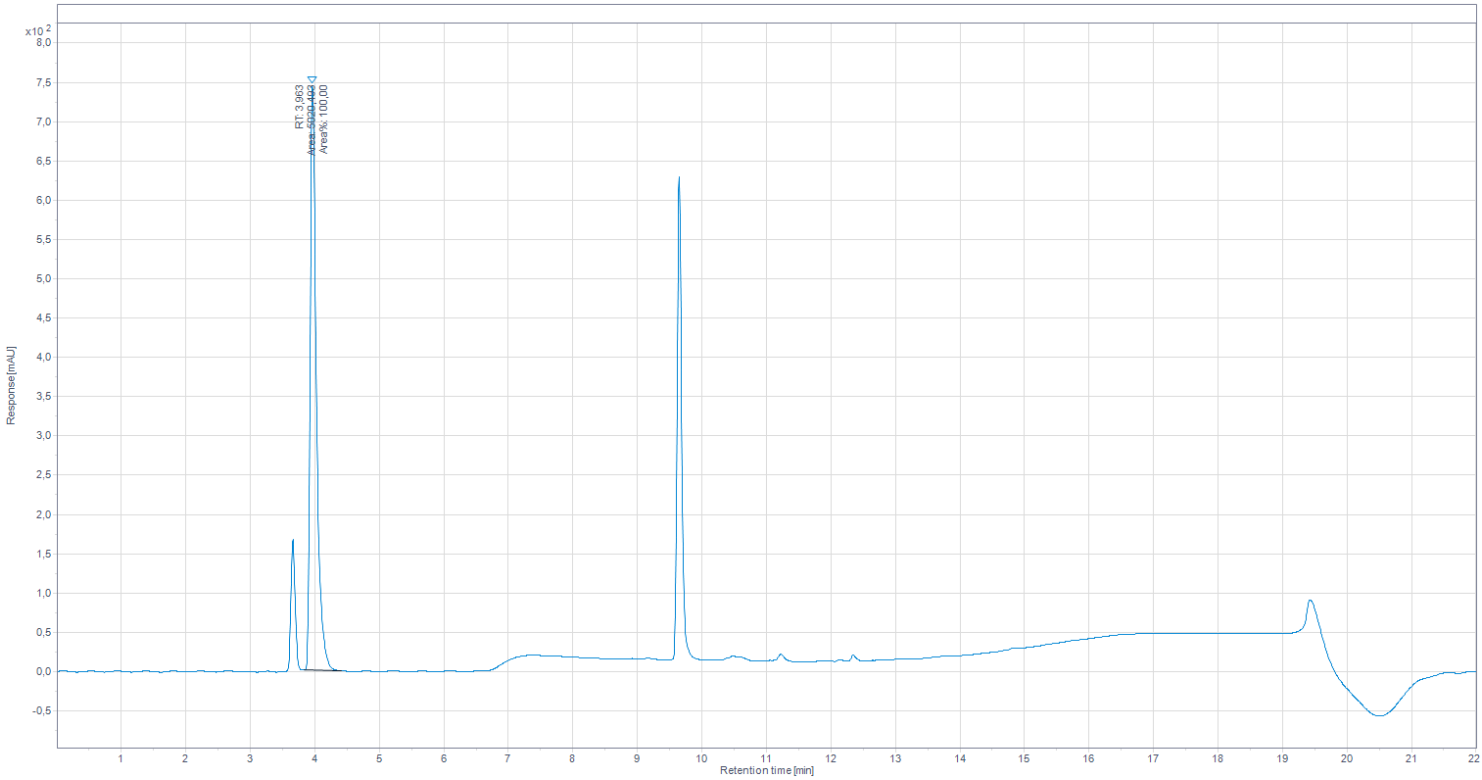

Password

7W54S2MH

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając

ANALIZA BIAŁEK

100013609

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
60min	5%	95%
62min	5%	95%

Password

7W54S2MH

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając